

INSTRUCTION MANUAL



KEPCO An ISO 9001 Company.

**KIT
219-0508**

CHASSIS SLIDES KIT NO. 219-0508

1. DESCRIPTION

This Kepco KIT contains the components required to install bottom-mount chassis slides on Kepco RA 19-4C Rack Adapters..

2. INSTALLATION OF CHASSIS SLIDES

2.1 MATERIAL SUPPLIED (SEE TABLE 1.)

TABLE 1. MATERIAL SUPPLIED

MATERIAL	QUANTITY
Slide, Kepco P/N 108-0458 (Accuride 3012590, modified)	2
Screw, 6-32 x 1/4 in. long, Kepco P/N 101-0458	4
Instruction Manual, Kit 219-0508	1

2.2 PROCEDURE (SEE FIGURES 1, 2, 3.)

1. Remove four feet from bottom of RA 19-4C chassis.
2. Attach slides (108-0458) to each side of rack adapter using four screws (101-0458) (see Figure 1). Locate the locking detent towards the rear of the chassis to ensure forward travel.
3. Attach slides to cabinet using mounting holes "A."


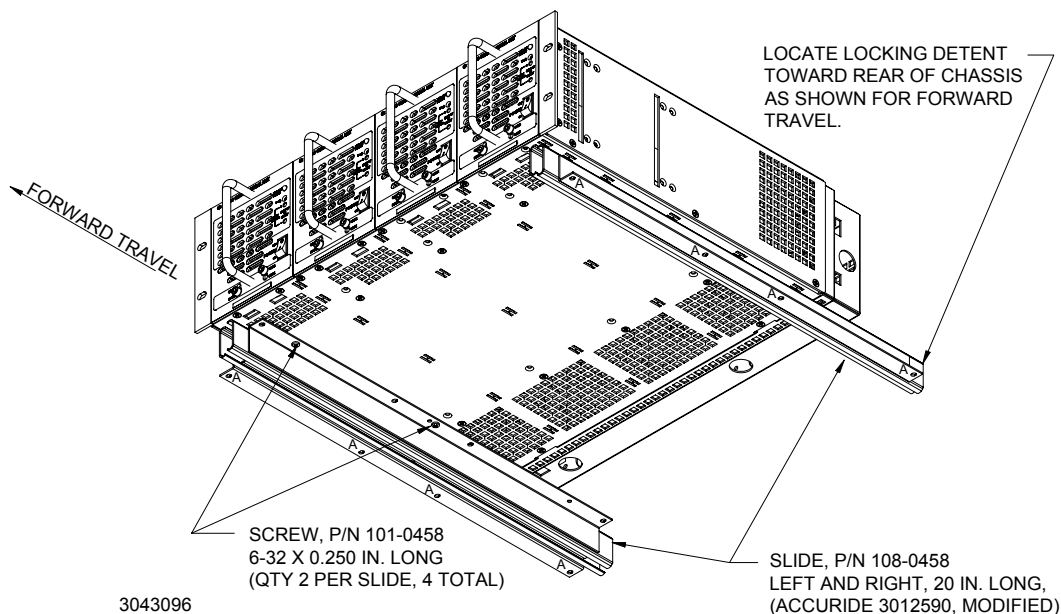



FIGURE 1. INSTALLING CHASSIS SLIDES ON RACK ADAPTER (3/4 VIEW OF BOTTOM)

KEPCO, INC. ● 131-38 SANFORD AVENUE ● FLUSHING, NY. 11352 U.S.A. ● TEL (718) 461-7000 ● FAX (718) 767-1102
<http://www.kepcopower.com> ● email: hq@kepcopower.com

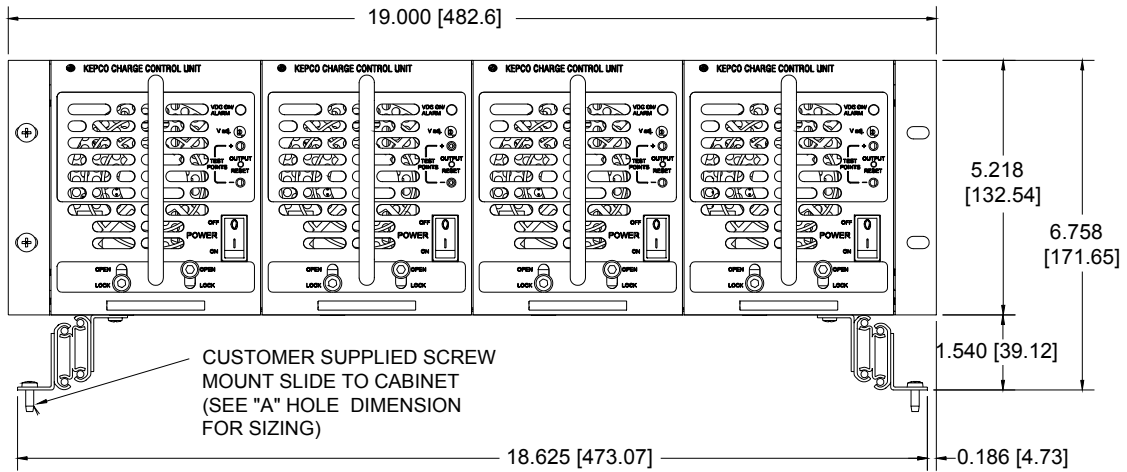

3043098 NOTES: 1. DIMENSIONS IN INCHES, DIMENSIONS IN BRACKETS ARE IN MILLIMETERS.
2. TOLERANCES ARE ± 0.015 [± 0.38] UNLESS OTHERWISE SPECIFIED.

FIGURE 2. INSTALLING CHASSIS SLIDES ON RACK ADAPTER (FRONT VIEW)

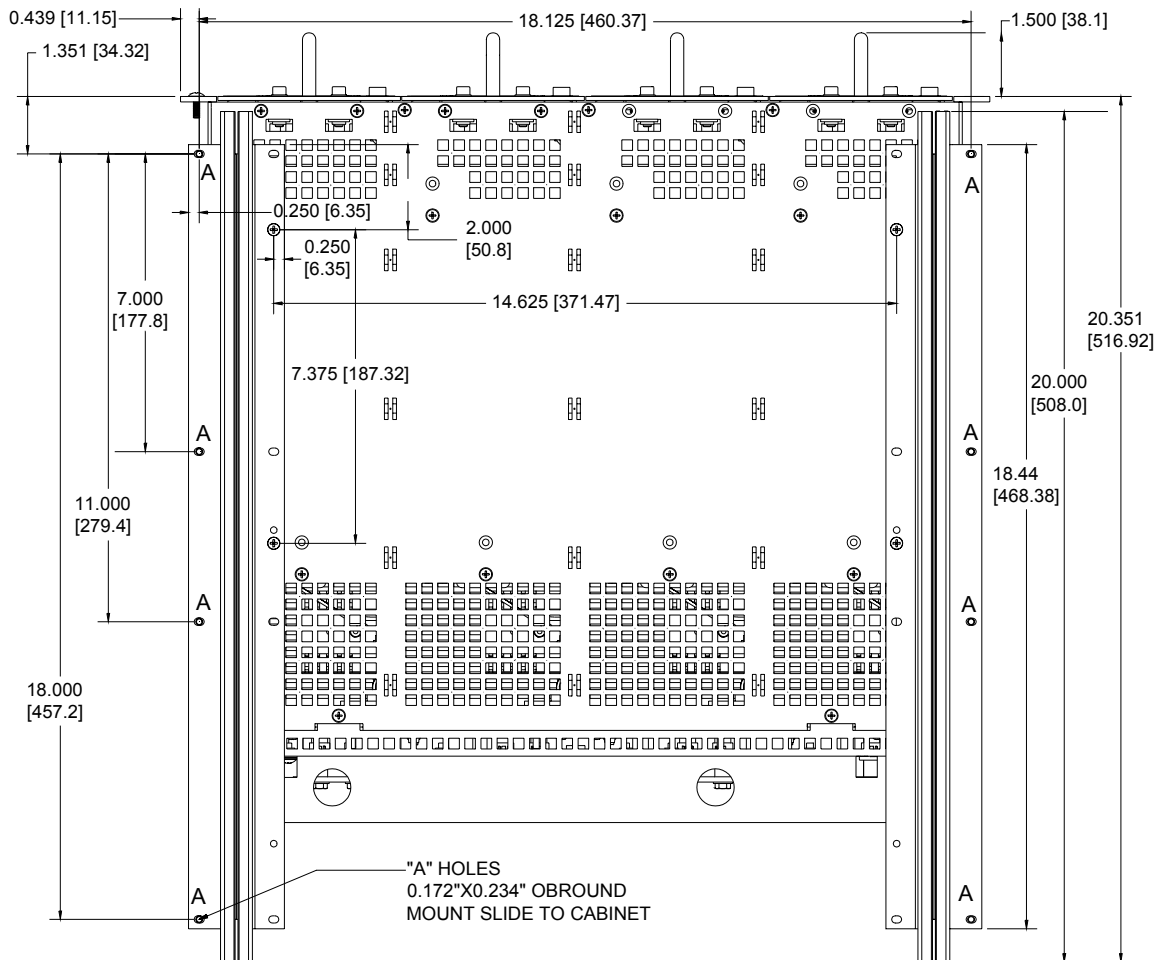

3043097 NOTES: 1. DIMENSIONS IN INCHES, DIMENSIONS IN BRACKETS ARE IN MILLIMETERS.
2. TOLERANCES ARE ± 0.015 [± 0.38] UNLESS OTHERWISE SPECIFIED.

FIGURE 3. INSTALLING CHASSIS SLIDES ON RACK ADAPTER (BOTTOM VIEW)

KEPCO, INC. ● 131-38 SANFORD AVENUE ● FLUSHING, NY. 11352 U.S.A. ● TEL (718) 461-7000 ● FAX (718) 767-1102
http://www.kepcopower.com ● email: hq@kepcopower.com