


INSTRUCTION SHEET



KEPCO An ISO 9001 Company.

RA 8-2

RA 8-2 RACK ADAPTER

I — DESCRIPTION.

This kit contains the hardware required to mount two PRM Size A-180, Size AA-280, Size C-300 or Size C-450 Series Power Supplies to a standard 19-inch equipment rack.

II — EQUIPMENT SUPPLIED

Table 1 lists the equipment supplied.

TABLE 1. EQUIPMENT SUPPLIED

Item	Quantity	Description	Kepeco P/N
Panel	1	Allows installation of Series A-180, AA-280, C-300 and C-450 PRM power supplies on standard 19-inch rack.	168-0037
Handle	2	Facilitates moving and installing rack adapter.	139-0103
Screw	4	Used to attach handle to panel (10-32 x 7/4, ST. FHP2).	101-0043
Ferrule	4	Used to reinforce handle to panel.	170-0001
Screw	8	Used to attach PRM power supply to panel (10-32 x 1-2, ST., THPH).	101-0040
Washer	8	Used to attach PRM power supply to panel (Lock, #10).	103-0134

III — ASSEMBLY

Mount each handle onto two ferrules (P/N 170-0001) and attach to the panel using four screws (P/N 101-0043) at mounting holes C (see Figure 1), Attach PRM power supplies to the panel using four screws (P/N 101-0029) and four washers (P/N 103-0068) for each power supply at mounting holes A.

IV — INSTALLATION

Mount the assembled rack adapter with the PRM power supplies attached to the 19-inch rack using hardware (not supplied) at mounting holes B.

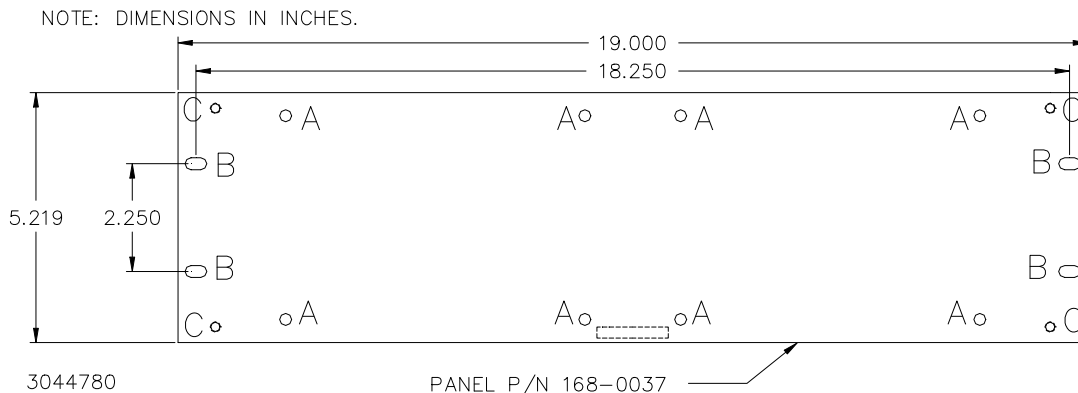


FIGURE 1. RACK ADAPTER RA 8-2